

## CLINICAL PAPER

# Miniaturized mechanical chest compressor: A new option for cardiopulmonary resuscitation<sup>☆</sup>

Giuseppe Ristagno<sup>a</sup>, Carlos Castillo<sup>a</sup>, Wanchun Tang<sup>a,b</sup>, Shijie Sun<sup>a,b</sup>, Joe Bisera<sup>a,b</sup>, Max Harry Weil<sup>a,b,c,\*</sup>

<sup>a</sup> Weil Institute of Critical Care Medicine, Rancho Mirage, CA, United States

<sup>b</sup> Keck School of Medicine of the University of Southern California, Los Angeles, CA, United States

<sup>c</sup> Northwestern University, Feinberg School of Medicine, Chicago, IL, United States

Received 1 November 2006; received in revised form 27 June 2007; accepted 2 July 2007

### KEYWORDS

Cardiac arrest;  
Cardiopulmonary  
resuscitation;  
Chest compression;  
Mechanical chest  
compressor;  
Coronary perfusion  
pressure;  
Myocardial function;  
Post-resuscitation  
survival

### Summary

**Aim of study:** After cardiac arrest, uninterrupted chest compressions with restoration of myocardial blood flow facilitates restoration of spontaneous circulation. We recognized that this may best be accomplished with a mechanical device and especially so during transport. We therefore sought to develop a lightweight, portable chest compressor which may be carried on the belt or attached to the oxygen tank typically carried on the back of the first response rescuer. A miniaturized pneumatic chest compressor (MCC) weighing less than 2 kg was developed and compared with a currently marketed “Michigan Thumper<sup>®</sup>”, which weighed 19 kg. We hypothesized that the 2 kg, low profile, portable device will be as effective as the standard pneumatic Thumper<sup>®</sup> for restoring circulation during CPR.

**Material and methods:** Ventricular fibrillation was electrically induced in 10 domestic male pigs weighing  $39 \pm 2$  kg, and untreated for 5 min. Animals were then randomized to receive chest compressions with either the MCC or the Thumper<sup>®</sup>. After 5 min of mechanical chest compression, defibrillation was attempted with a 150 J biphasic shock. Coronary perfusion pressure (CPP) and end tidal PCO<sub>2</sub> (EtPCO<sub>2</sub>) were measured by conventional techniques together with right carotid artery blood flow (CBF).

**Results:** Four of five animals compressed with the Thumper<sup>®</sup> and each animal compressed with the MCC were successfully resuscitated. No significant differences in CPP, EtPCO<sub>2</sub>, CBF and post-resuscitation myocardial function were observed between groups. Resuscitated animals survived for more than 72 h without neurological impairment.

**Conclusion:** The low profile, 2 kg miniaturized chest compressor is as effective as the conventional Thumper<sup>®</sup> in an experimental model of CPR.

© 2007 Elsevier Ireland Ltd. All rights reserved.

<sup>☆</sup> A Spanish translated version of the summary of this article appears as Appendix in the final online version at [10.1016/j.resuscitation.2007.07.004](http://10.1016/j.resuscitation.2007.07.004).

\* Corresponding author at: Weil Institute of Critical Care Medicine, 35100 Bob Hope Drive, Rancho Mirage, CA 92270, United States. Tel.: +1 760 778 4911; fax: +1 760 778 3468.

E-mail address: [weilm@weiliccm.org](mailto:weilm@weiliccm.org) (M.H. Weil).

## Introduction

Cardiovascular disease continues to be the leading cause of death and more than 400,000 Americans and 700,000 Europeans are victim of cardiac arrests each year.<sup>1</sup> Despite major efforts to improve outcomes from cardiac arrest, fewer than 5% of victims are hospital survivors.<sup>2–5</sup> Both in heavily populated larger cities and in sparsely populated rural communities, delayed response by emergency medical services compromises outcomes such that survival is even more disappointing, namely as low as 1%.<sup>6,7</sup>

There is now evidence that the highest priority of intervention is to re-establish systemic blood flow promptly by external chest compression and thereby achieve and maintain threshold levels of coronary and cerebral perfusion. Accordingly, effective, consistent and uninterrupted chest compression is now designated as the primary intervention for management of cardiac arrest. Both survival and neurological recovery are contingent upon initiating chest compression within less than 5 min.<sup>8–10</sup> Accordingly, bystander initiated chest compressions by minimally trained, non-professional rescuers subsequently supported by well organized professional emergency medical providers have significantly increased survival from out-of-hospital cardiac arrest.<sup>11–13</sup>


In addition to the benefits of prompt intervention, it is also the quality of chest compressions delivered in both in- and out-of-hospital settings, which has proven to be a determinant of outcomes. Even well-trained professional providers cannot maintain effective chest compression for intervals that exceed 2 min.<sup>14–17</sup> This limitation is in addition to the documented inconsistency of depth and rate of compressions.<sup>18–20</sup> The challenges are even greater during evacuation and transport of victims. Therefore, the option of using mechanical devices is attractive. Mechanical chest compression potentially overcomes operator fatigue, slow rates of compression, and inadequate depth of compression. A mechanical compressor would also allow for the delivery of an electrical shock without interruption of manual compression for the protection of the rescuer.

The present study in a porcine model was therefore undertaken to compare the effectiveness of a newly developed miniaturized pneumatic chest compressor (MCC) with that of a conventional and commercially available compression device (Figure 1). The MCC was so designed that it may be carried on the belt or attached to the oxygen gas tank carried routinely by the professional rescuer. It is pneumatically powered with oxygen or compressed air. In Table 1, the principal features of the two devices are compared. The biomedical engineering details of design, construction, and pneumatic operation of the MCC will be addressed in detail in a separate medical engineering publication.

We tested the hypothesis that such a lightweight device would be as effective as a current standard, the Thumper® (Model 1004, Michigan Instruments, Grand Rapids, MI), for restoring circulation during CPR after cardiac arrest.

## Materials and methods

All animals received humane care in compliance with the "Principles of Laboratory Animal Care" formulated by the

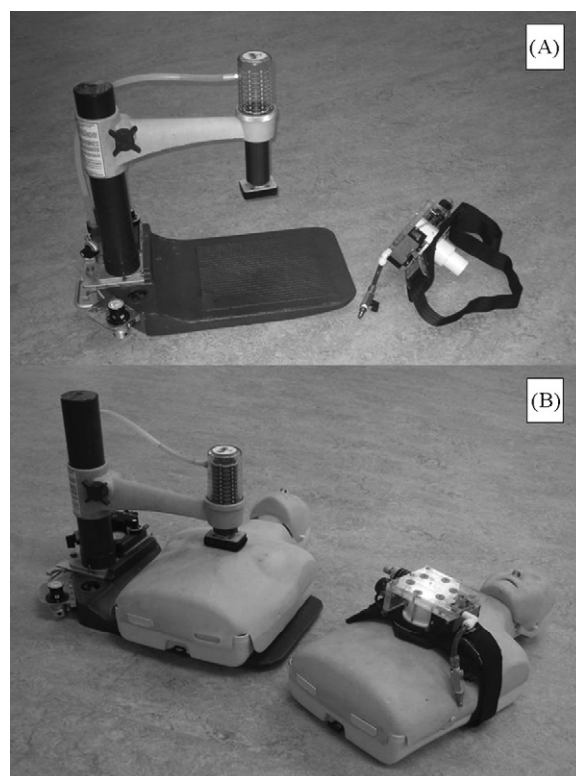

**Figure 1** (A) The Michigan Thumper® shown on the left and the MCC on the right. (B) The Michigan Thumper® applied to a manikin on the left and the MCC applied to a manikin on the right.

National Society for Medical Research and the *Guide for the Care and Use of Laboratory Animals* prepared by the Institute of Laboratory Animal Resources and published by the National Institutes of Health (NIH publication 86-32, revised 1985). The protocol was approved by the Institutional Animal Care and Use Committee of the Weil Institute of Critical Care Medicine. The animal laboratories of the Weil Institute are fully accredited by American Association for Accreditation of Laboratory Animal Care (AAALAC) International.

**Table 1** A comparison of the features of the two chest compression devices

	MCC	Thumper®
Weight (kg)	2	19
Length (cm)	35	61
Width (cm)	15	30
Height (cm)	9	139.5
Force at pneumatic pressure of 50 psi (kg)	48	55
Gas consumption (L/min)	46	45
Compression rate (compressions/min)	90 ± 5	90 ± 5
Maximal piston descent (cm)	10	10

## Animal preparation

Ten male domestic pigs weighing  $39 \pm 2$  kg were fasted overnight except for free access to water. Anesthesia was initiated by an intramuscular injection of ketamine (20 mg/kg) and completed by ear vein injection of sodium pentobarbital (30 mg/kg). Additional doses of sodium pentobarbital (8 mg/kg) were injected at intervals of approximately 1 h to maintain anesthesia. A cuffed tracheal tube was advanced into the trachea. Animals were mechanically ventilated with a volume-controlled ventilator (Model MA-1, Puritan-Bennett, Carlsbad, CA) with a tidal volume of 15 mL/kg, peak flow of 40 L/min, and  $\text{FiO}_2$  of 0.21. End-tidal  $\text{PCO}_2$  ( $\text{EtPCO}_2$ ) was monitored with an infrared capnometer (Model NPB-75, Nellcor Puritan Bennett Inc., Pleasanton, CA). Respiratory frequency was adjusted to maintain  $\text{EtPCO}_2$  between 35 and 40 mmHg. For measurement of left ventricular function, a transesophageal echocardiographic transducer was advanced from the incisor teeth into the esophagus for a distance of approximately 35 cm. For measurement of mean aortic pressure (MAP), a fluid-filled catheter was advanced from the right femoral artery into the thoracic aorta. For the measurements of right atrial pressure (RAP), mean pulmonary artery pressure (MPAP), and thermodilution cardiac output ( $\text{CO}_{\text{TD}}$ ), a 7-Fr pentaluminal, thermodilution-tipped catheter was advanced from the right femoral vein and flow directed into the pulmonary artery. Carotid blood flow (CBF) was continuously measured with the aid of a flowprobe (Ultrasonic Blood Flow Meter, T101, Transonic Systems Inc., Ithaca, NY) positioned around the right common carotid artery. For inducing VF, a 5-Fr pacing catheter (EP Technologies, Inc., Mountain View, CA) was advanced from the right subclavian vein into the right ventricle. The position of catheters was confirmed by characteristic pressure morphology and/or fluoroscopy. The pacing catheter was removed after onset of VF. The piston of the compressor was positioned in the midline at the level of the fifth interspace and this locus was defined prior to randomization. Repositioning of the devices was not required because they were stable once positioned. Precordial compression was started with either the Thumper® or the MCC. The chest compressors were programmed to provide equal compression–relaxation intervals, i.e. a 50% duty cycle. Coincident with the start of precordial compression, the animals were ventilated asynchronously with a tidal volume of 15 mL/kg and  $\text{FiO}_2$  of 1.0 and with a rate of 10 breaths per min.

## Experimental procedures

Before inducing cardiac arrest, the animals were randomized by the sealed envelope method to receive chest compression by either of the two piston-driven devices. VF was induced with 1–2 mA alternating current delivered to the endocardium of the right ventricle. Mechanical ventilation was discontinued after onset of VF. After 5 min of untreated VF, mechanical chest compression with one of the two devices was begun. Animals were ventilated simultaneously with 100% oxygen for the ensuing 5 min. Electrical defibrillation was then attempted with a sin-

gle biphasic 150 J electrical shock, delivered between the conventional right infraclavicular electrode and the apical electrode with a Heartstart XL defibrillator (Philips Medical Systems, Andover, MA). If spontaneous circulation was not restored, mechanical chest compressions with the same compressor and ventilation were resumed and continued for 2 min before a subsequent defibrillation attempt. The same resuscitation procedure was continued until successful resuscitation or for a maximum of 15 min. No vasopressor drugs were used. The animals were regarded as successfully resuscitated if an organized cardiac rhythm with MAP of more than 60 mmHg persisted for an interval of 5 min or more. Anesthesia was continued and animals were monitored for an additional 4 h. With the aid of an image intensifier and fluoroscopy, we visualized the bony thorax and counted the number of fractured ribs. Catheters were then removed, wounds were surgically repaired, and animals were extubated before they were returned to their cages. The animals were then observed for an additional 68 h. At the end of the 72-h post-resuscitation observation interval, animals were reanesthetized with ketamine and pentobarbital. Echo-Doppler measurements of myocardial functions were then repeated. Animals were then sacrificed painlessly with an intravenous injection of 150 mg/kg pentobarbital. Autopsy was performed routinely for documentation of potential injuries to the thoracic and abdominal viscera occurring during CPR, including fractured ribs, or due to obfuscating disease.

## Measurements

Hemodynamic data,  $\text{EtPCO}_2$ , and ECG were measured continuously and recorded on a PC-based data acquisition system supported by CODAS hardware/software as described previously.<sup>21</sup> Coronary perfusion pressure (CPP) was digitally computed from the differences in time-coincident diastolic aortic and right atrial pressures and displayed in real time. Arterial and mixed venous blood gases, hemoglobin and oxyhemoglobin were measured on 200  $\mu\text{L}$  aliquots of blood with a stat profile analyzer (ULTRA C, Nova Biomedical Corporation, Waltham, MA) adapted for porcine blood. These measurements were obtained at 15 min before inducing cardiac arrest and at 4 min after starting chest compression. Cardiac output was measured by conventional thermodilution techniques after injection of 5 mL of saline maintained at 2 °C. Echocardiographic measurements were obtained with the aid of a S7-t3 mini-multi, transesophageal echocardiographic transducer (Model HD11XE, Philips Medical Systems, Eindhoven, Netherlands). Long axis two-chamber views were obtained. Left ventricular end-systolic and end-diastolic volumes were calculated by the method of discs, as previously described.<sup>21</sup> From these, stroke volumes (SV), ejection fractions (EF) and fractional area change (FAC) were computed. Measurements were obtained at baseline and at hourly intervals thereafter for a total of 4 h. These measurements were repeated at 72 h following resuscitation to quantify myocardial function. A neurological alertness score (NAS), developed by our group<sup>22</sup> was used for evaluating neurological recovery at 24, 48, and 72 h.


## Statistical analyses

The independent variables were the two mechanical chest compressors, the Thumper® and the MCC. The dependent variables were initial resuscitation; CPP, EtPCO<sub>2</sub> and CBF during chest compression; numbers of shocks delivered before restoration of spontaneous circulation (ROSC) and incidence of recurrent VF. Additional independent variables included duration of CPR; numbers of fractured ribs; post-resuscitation myocardial function including left ventricular SV, EF and FAC; post-resuscitation neurological recovery; and post-resuscitation duration of survival. For measurement between groups, ANOVA with Scheffe's method for multiple comparisons was used. When the dependent variable was categorical such as 24, 48, and 72 h survival, Fisher's exact test was used. Values are reported as mean ± standard deviation. A *p* value of <0.05 was regarded as significant.

## Results

There were no differences in the baseline values blood gas measurements, heart rate (HR), MAP, EtPCO<sub>2</sub>, RAP, MPAP and CO<sub>TD</sub>, between the two groups (Table 2). In each animal treated with the MCC device, ROSC was achieved with only a single shock (Table 3). Four of the five animals treated with the Thumper® achieved ROSC.

During chest compression, we observed no significant differences in CPP, EtPCO<sub>2</sub>, CBF (Figure 2) or in the arterial blood concentrations of lactate (Figure 3) between the two groups. Both CPP and CBF were numerically greater with the MCC, but the differences were only of borderline statistical significance. We observed a numerical but not statistically

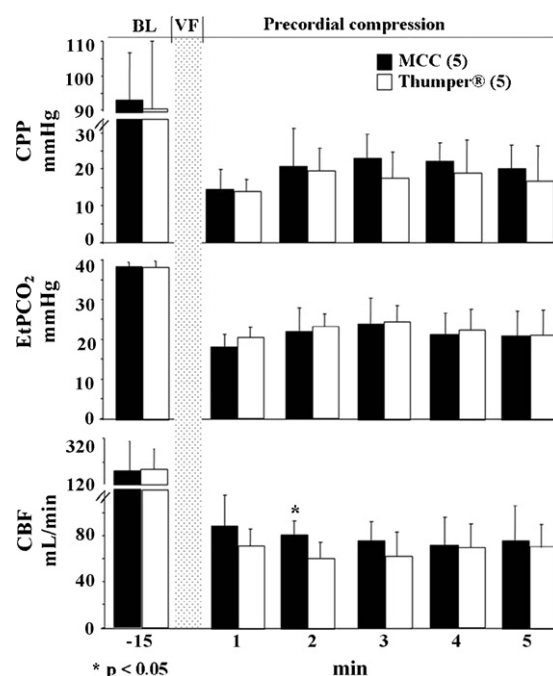

**Figure 2** A comparison of coronary perfusion pressures (CPP), end-tidal PCO<sub>2</sub> (EtPCO<sub>2</sub>) and carotid blood flows (CBF) at baseline (BL) and during precordial compression. Mean ± S.D.; \**p* < 0.05.

significant lower incidence of fractured ribs with the MCC (Figure 3).

Each resuscitated animal survived for 72 h with full neurological recovery. No differences in baseline or post-resuscitation thermodilution cardiac output, MAP or


**Table 2** Baseline measurements (mean ± S.D.)

	MCC (5)	Thumper® (5)	<i>p</i> (MCC vs. Thumper®)
Animal weight (kg)	39.8 ± 1.8	37.6 ± 2.3	0.13
PaO <sub>2</sub> /FiO <sub>2</sub>	410 ± 72	414 ± 89	0.93
LAC (mmol/L)	1.2 ± 0.7	0.8 ± 0.3	0.28
HR (beats/min)	140 ± 44	123 ± 16	0.44
MAP (mmHg)	107 ± 7	108 ± 13	0.91
RAP (mmHg)	3 ± 1	4 ± 2	0.41
MPAP (mmHg)	21 ± 2	20 ± 3	0.65
CO <sub>TD</sub> (L/min)	8 ± 1.2	7 ± 0.8	0.15

PaO<sub>2</sub> = arterial partial pressure of oxygen; FiO<sub>2</sub> = inspiratory fraction of oxygen; LAC = arterial blood lactate; HR = heart rate; CO<sub>TD</sub> = thermodilution cardiac output.

**Table 3** Resuscitation outcomes (mean ± S.D.)

	MCC	Thumper®	<i>p</i> (MCC vs. Thumper®)
Resuscitated	5/5	4/5	0.3
Number of shocks prior to ROSC	1	1.25 ± 0.5	0.29
Incidence of recurrent of VF	2 ± 2.8	0.5 ± 1	0.35
Duration of CPR prior to ROSC	306 ± 11	334 ± 76	0.39

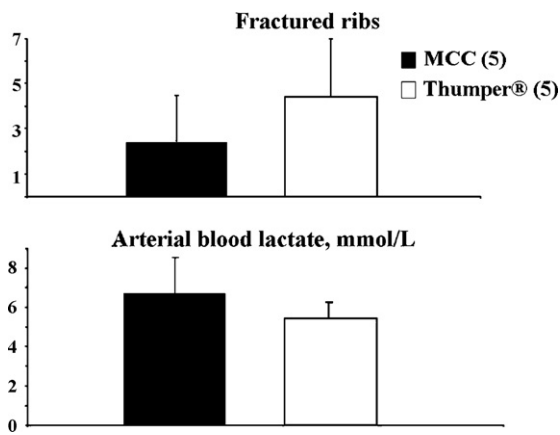

**Figure 3** A comparison of the number of fractured ribs produced by chest compressions with the two devices and arterial blood lactate concentration measured at 4 min after start of precordial compression. Mean  $\pm$  S.D.

echocardiographically measured myocardial function were observed between the two groups (Table 4).

## Discussion

The present study documented that the new miniaturized chest compressor was as effective as the Thumper® with respect to increases in CPP and EtPCO<sub>2</sub> during chest compressions. The MCC generated marginally greater CBF. There were no statistically significant differences in outcomes with respect to the success of initial resuscitation, post-resuscitation myocardial function, post-resuscitation neurological recovery, and 72 h survival. Accordingly, the goal of our effort was achieved, namely equivalency of the effectiveness and outcomes when the two compression devices were compared.

Current guidelines strongly recommend chest compression to restore blood flow to vital organs as the primary intervention after “sudden death”, especially when the duration of untreated cardiac arrest is greater than 5 min.<sup>8</sup> Following prolonged untreated cardiac arrest progressive energy imbalances develop since chest compression produces less than 50% of pre-arrest stroke volumes.<sup>23–26</sup> However, threshold levels of myocardial and cerebral blood flows are restored such as to minimize ischemic myocardial and cerebral ischemic injury.<sup>27</sup> CPP is a key predictor of the likelihood of successful ROSC and both the Thumper® and the MCC consistently increased CPP to levels that exceeded the threshold of 15 mmHg for successful ROSC.<sup>28–30</sup> EtPCO<sub>2</sub>, which has also emerged as an indirect measure of pulmonary blood flow and therefore cardiac output produced by chest compression, continuously exceeded the threshold level of approximately 15 mmHg, which is predictive of successful resuscitation.<sup>31–34</sup>

Several new devices have recently been introduced to facilitate mechanical chest compression. Both the LUCAS (Jolife, Medtronic, Sweden) and the AutoPulse (Revivant Corporation, CA, USA) have demonstrated equivalency and potentially even greater effectiveness than manual chest compression.<sup>35–38</sup> In each instance, however, the weight of the devices ranges from 6.5 to 12.2 kg and width from

**Table 4** Post-resuscitation hemodynamic measurements (mean  $\pm$  S.D.)

Hours	MCC	Thumper®	<i>p</i> (MCC vs. Thumper®)
Stroke volume (mL)			
BL	29 $\pm$ 11	30 $\pm$ 12	0.91
PR 1	19 $\pm$ 6	23 $\pm$ 4	0.31
PR 2	22 $\pm$ 4	26 $\pm$ 5	0.29
PR 3	23 $\pm$ 4	25 $\pm$ 6	0.53
PR 4	27 $\pm$ 7	25 $\pm$ 6	0.68
PR 72	31 $\pm$ 14	27 $\pm$ 2	0.77
Ejection fraction (%)			
BL	64 $\pm$ 6	61 $\pm$ 3	0.27
PR 1	54 $\pm$ 7	55 $\pm$ 6	0.78
PR 2	54 $\pm$ 4	57 $\pm$ 7	0.34
PR 3	54 $\pm$ 3	58 $\pm$ 2	0.11
PR 4	56 $\pm$ 4	61 $\pm$ 8	0.24
PR 72	63 $\pm$ 2	62 $\pm$ 3	0.77
Fractional area change (%)			
BL	51 $\pm$ 4	47 $\pm$ 5	0.59
PR 1	36 $\pm$ 6	37 $\pm$ 10	0.76
PR 2	38 $\pm$ 2	39 $\pm$ 6	0.77
PR 3	40 $\pm$ 3	42 $\pm$ 3	0.39
PR 4	42 $\pm$ 3	43 $\pm$ 7	0.81
PR 72	47 $\pm$ 8	48 $\pm$ 4	0.64
CO <sub>TD</sub> (L/min)			
BL	8 $\pm$ 1.2	7 $\pm$ 0.8	0.15
PR 1	7.2 $\pm$ 1	6 $\pm$ 1	0.12
PR 2	7.5 $\pm$ 1.4	5.8 $\pm$ 1.5	0.13
PR 3	7.2 $\pm$ 1.5	5.4 $\pm$ 0.9	0.07
PR 4	6.9 $\pm$ 1.3	6.2 $\pm$ 1.4	0.41
MAP (mmHg)			
BL	107 $\pm$ 7	108 $\pm$ 13	0.91
PR 1	104 $\pm$ 11	94 $\pm$ 4	0.14
PR 2	107 $\pm$ 11	101 $\pm$ 11	0.47
PR 3	107 $\pm$ 8	103 $\pm$ 6	0.47
PR 4	111 $\pm$ 3	108 $\pm$ 4	0.29

Baseline (BL) measurements on five animals per group. Post-resuscitation (PR) measurements on five animals with the MCC and four animals with the Thumper®; CO<sub>TD</sub> = thermodilution cardiac output.

44 to 46 cm. These physical dimensions compromise portability. The MCC weighs <2 kg and is only 15 cm in width. The MCC complies with the inventors’ intent, namely that it may be carried without significant burden by the first response professional rescuer (Figure 4) such as to facilitate prompt start of mechanical chest compression on arrival. The MCC is anchored in position on the patient’s thorax regardless of the victim’s body position, a major advantage during evacuation through stairways and around corners.

In addition, to its modest dimensions and weight, the MCC therefore fulfils the need of a mechanical device for both early implementation and uninterrupted, effective chest compressions. The advantages of size and weight also allow for chest compression during ambulance transport and transport through hospital hallways and elevators. Perhaps most important, effective and uninterrupted precordial compres-



**Figure 4** The MCC worn on the belt of the professional rescuer.

sion provided by mechanical compressors is not limited by operator fatigue.

We recognize limitations in the interpretation of our findings. The studies were conducted in healthy animals and therefore in the absence of underlying diseases or injuries that are causative of cardiac arrest. The investigators were not blinded to the intervention and, accordingly, the possibility of observer bias in the physical application of the mechanical chest compressors to the chest of the animal is not excluded although the location of the piston was the same for both groups. The close relationship among measurements of CPP, EtPCO<sub>2</sub>, and CBF during chest compression provides additional evidence. Finally, the present study demonstrates equivalency with an approved device but without comparison to conventional manual chest compressions. However, the evidence that with manual compression, rescuer fatigue, interruption of chest compression for the delivery of defibrillating shock and the difficulty of manual compression during transport, would provide persuasive evidence to the contrary.

## Conclusions

The miniaturized mechanical chest compressor represents a new option for CPR. It is as effective as the conven-

tional Thumper® with respect to increases in CPP, EtCO<sub>2</sub> and carotid blood flow during chest compressions. The MCC has the advantage of lightweight and compact dimensions so that it may be carried routinely on the belt of first response rescuers and allow for uninterrupted CPR during transport.

## Conflict of interest

No conflicts of interest are reported. No financial benefits to the researchers are reported. All benefits of all inventions of the Weil Institute of Critical Care Medicine are totally reserved for research support and none accrue to the personal benefit of any of the inventors or researchers.

## Acknowledgments

This study was supported in part by a grant in aid for the American Heart Association, Dallas, TX.

The abstract of this paper was accepted for presentation at the American Heart Association 2006, Resuscitation Science Symposium and first author was the recipient of a Resuscitation Science Young Investigator Award.

## References

1. International Liaison Committee on Resuscitation. Part 2. Adult basic life support. *Resuscitation* 2005;67(2/3):187–201.
2. Sanders AB, Ewy GA. Cardiopulmonary resuscitation in the real world: when will the guidelines get the message? *JAMA* 2005;293(3):363–5.
3. Nichol G, Stiell IG, Laupacis A, Pham B, De Maio VJ, Wells GA. A cumulative meta-analysis of the effectiveness of defibrillator-capable emergency medical services for victims of out-of-hospital cardiac arrest. *Ann Emerg Med* 1999;34:517–25.
4. Engdahl J, Bang A, Lindqvist J, Herlitz J. Time trends in long-term mortality after out-of-hospital cardiac arrest, 1980–1998, and predictors for death. *Am Heart J* 2003;145:826–33.
5. Eisenberg MS, Horwood BT, Cummins RO, Reynolds-Haertke R, Hearne TR. Cardiac arrest and resuscitation: a tale of 29 cities. *Ann Emerg Med* 1990;19:179–86.
6. Becker LB, Ostrander MP, Barrett J, Kondos GT. Outcome of CPR in a large metropolitan area—where are the survivors? *Ann Emerg Med* 1991;20:355–61.
7. Caffrey SL, Willoughby PJ, Pepe PE, Becker LB. Public use of automated external defibrillators. *N Engl J Med* 2002;347(16):1242–7.
8. International Liaison Committee on Resuscitation. Part 3. Defibrillation. *Resuscitation* 2005;67(2/3):203–11.
9. Wik L, Hansen TB, Fylling F, et al. Delaying defibrillation to give basic cardiopulmonary resuscitation to patients with out-of-hospital ventricular fibrillation. *JAMA* 2003;289(11):1389–95.
10. Cobb LA, Fahrenbruch CE, Walsh TR, et al. Influence of cardiopulmonary resuscitation prior to defibrillation in patients with out-of-hospital ventricular fibrillation. *JAMA* 1999;281:1182–8.
11. Larsen MP, Eisenberg MS, Cummins RO, Hallstrom AP. Predicting survival from out-of-hospital cardiac arrest: a graphic model. *Ann Emerg Med* 1993;22:1652–8.
12. Rea TD, Eisenberg MS, Culley LL, Becker L. Dispatcher-assisted cardiopulmonary resuscitation and survival in cardiac arrest. *Circulation* 2001;104(21):2513–6.
13. White RD. Optimal access to — response by — public and voluntary services, including the role of bystanders and fam-

- ily members, in cardiopulmonary resuscitation. *New Horizons* 1997;5(2):153–7.
14. Ashton A, McCluskey A, Gwinnutt GL, Keenan AM. Effect of rescuer fatigue on performance of continuous external chest compressions over 3 min. *Resuscitation* 2002;55(2):151–5.
  15. Ochoa FJ, Ramalle-Gomara E, Lisa V, Saralegui I. The effect of rescuer fatigue on the quality of chest compressions. *Resuscitation* 1998;37(3):149–52.
  16. Hightower D, Thomas SH, Stone CK, Dunn K, March JA. Decay in quality of closed-chest compressions over time. *Ann Emerg Med* 1995;26(3):300–3.
  17. Plaisance P, Adnet F, Vicaut E, et al. Benefit of active compression–decompression cardiopulmonary resuscitation as prehospital advanced cardiac life support: a randomized multicenter study. *Circulation* 1997;95:955–61.
  18. Abella BS, Alvarado JP, Myklebust H, et al. Quality of cardiopulmonary resuscitation during in-hospital cardiac arrest. *JAMA* 2005;293:305–10.
  19. Wik L, Kramer-Johansen J, Myklebust H, et al. Quality of cardiopulmonary resuscitation during out-of-hospital cardiac arrest. *JAMA* 2005;293:299–304.
  20. Abella BS, Sandbo N, Vassilatos P, et al. Chest compression rates during cardiopulmonary resuscitation are suboptimal. *Circulation* 2005;111:428–34.
  21. Tang W, Weil MH, Sun SJ, et al. The effects of biphasic and conventional monophasic defibrillation on postresuscitation myocardial function. *J Am Coll Cardiol* 1999;34(3):815–22.
  22. Tang W, Weil MH, Sun S, et al. A comparison of biphasic and monophasic waveform defibrillation after prolonged ventricular fibrillation. *Chest* 2001;120:948–54.
  23. Johnson BA, Weil MH, Tang W, Noc M, McKee D, McCandless D. Mechanisms of myocardial hypercarbic acidosis during cardiac arrest. *J Appl Physiol* 1995;78(4):1579–84.
  24. Kern KB, Garewal HS, Sanders AB, et al. Depletion of myocardial adenosine triphosphate during prolonged untreated ventricular fibrillation: effect on defibrillation success. *Resuscitation* 1990;20:221–9.
  25. Shaffner DH, Eleff MS, Koehler RC, Traystman RJ. Effect of the no-flow interval and hypothermia on cerebral blood flow and metabolism during cardiopulmonary resuscitation in dogs. *Stroke* 1998;29:2607–15.
  26. Klouche K, Weil MH, Sun S, Tang W, Povoas H, Bisera J. Stroke volumes generated by precordial compression during cardiac resuscitation. *Crit Care Med* 2002;30:2626–31.
  27. Herlitz J, Ekstrom L, Wennerblom B, Axelsson A, Bang A, Holmberg S. Effects of bystander initiated cardiopulmonary resuscitation on ventricular fibrillation and survival after witnessed cardiac arrest outside hospital. *Br Heart J* 1994;72:408–12.
  28. Paradis NA, Martin GB, Rivers EP, et al. Coronary perfusion pressure and the return of spontaneous circulation in human cardiopulmonary resuscitation. *JAMA* 1990;263:1106–13.
  29. Sanders AB, Ogle M, Ewy GA. Coronary perfusion pressure during cardiopulmonary resuscitation. *Am J Emerg Med* 1985;2:11–4.
  30. Noc M, Weil MH, Tang W, Turner T, Fukui M. Mechanical ventilation may not be essential for initial cardiopulmonary resuscitation. *Chest* 1995;108:821–7.
  31. Weil MH, Bisera J, Trevino RP, Rackow EC. Cardiac output and end-tidal carbon dioxide. *Crit Care Med* 1985;13:907–9.
  32. Falk JL, Rackow EC, Weil MH. End-tidal carbon dioxide concentration during cardiopulmonary resuscitation. *N Engl J Med* 1988;318:607–11.
  33. Grmec S, Klemen P. Does the end-tidal carbon dioxide (EtCO<sub>2</sub>) concentration have prognostic value during out-of-hospital cardiac arrest? *Eur J Emerg Med* 2001;8(4):263–9.
  34. Cantineau JP, Lambert Y, Merckx P, et al. End-tidal carbon dioxide during cardiopulmonary resuscitation in humans presenting mostly with asystole: a predictor of outcome. *Crit Care Med* 1996;24(5):791–6.
  35. Steen S, Sjoberg T, Olsson P, Young M. Treatment of out-of-hospital cardiac arrest with LUCAS, a new device for automatic mechanical compression and active decompression resuscitation. *Resuscitation* 2005;67(1):25–30.
  36. Rubertsson S, Karlsten R. Increased cortical cerebral blood flow with LUCAS; a new device for mechanical chest compressions compared to standard external compressions during experimental cardiopulmonary resuscitation. *Resuscitation* 2005;65(3):357–63.
  37. Hallstrom A, Rea TD, Sayre MR, et al. Manual chest compression vs. use of an automated chest compression device during resuscitation following out-of-hospital cardiac arrest: a randomized trial. *JAMA* 2006;295(22):2620–8.
  38. Ong ME, Ornato JP, Edwards DP, et al. Use of an automated, load-distributing band chest compression device for out-of-hospital cardiac arrest resuscitation. *JAMA* 2006;295(22):2629–37.